

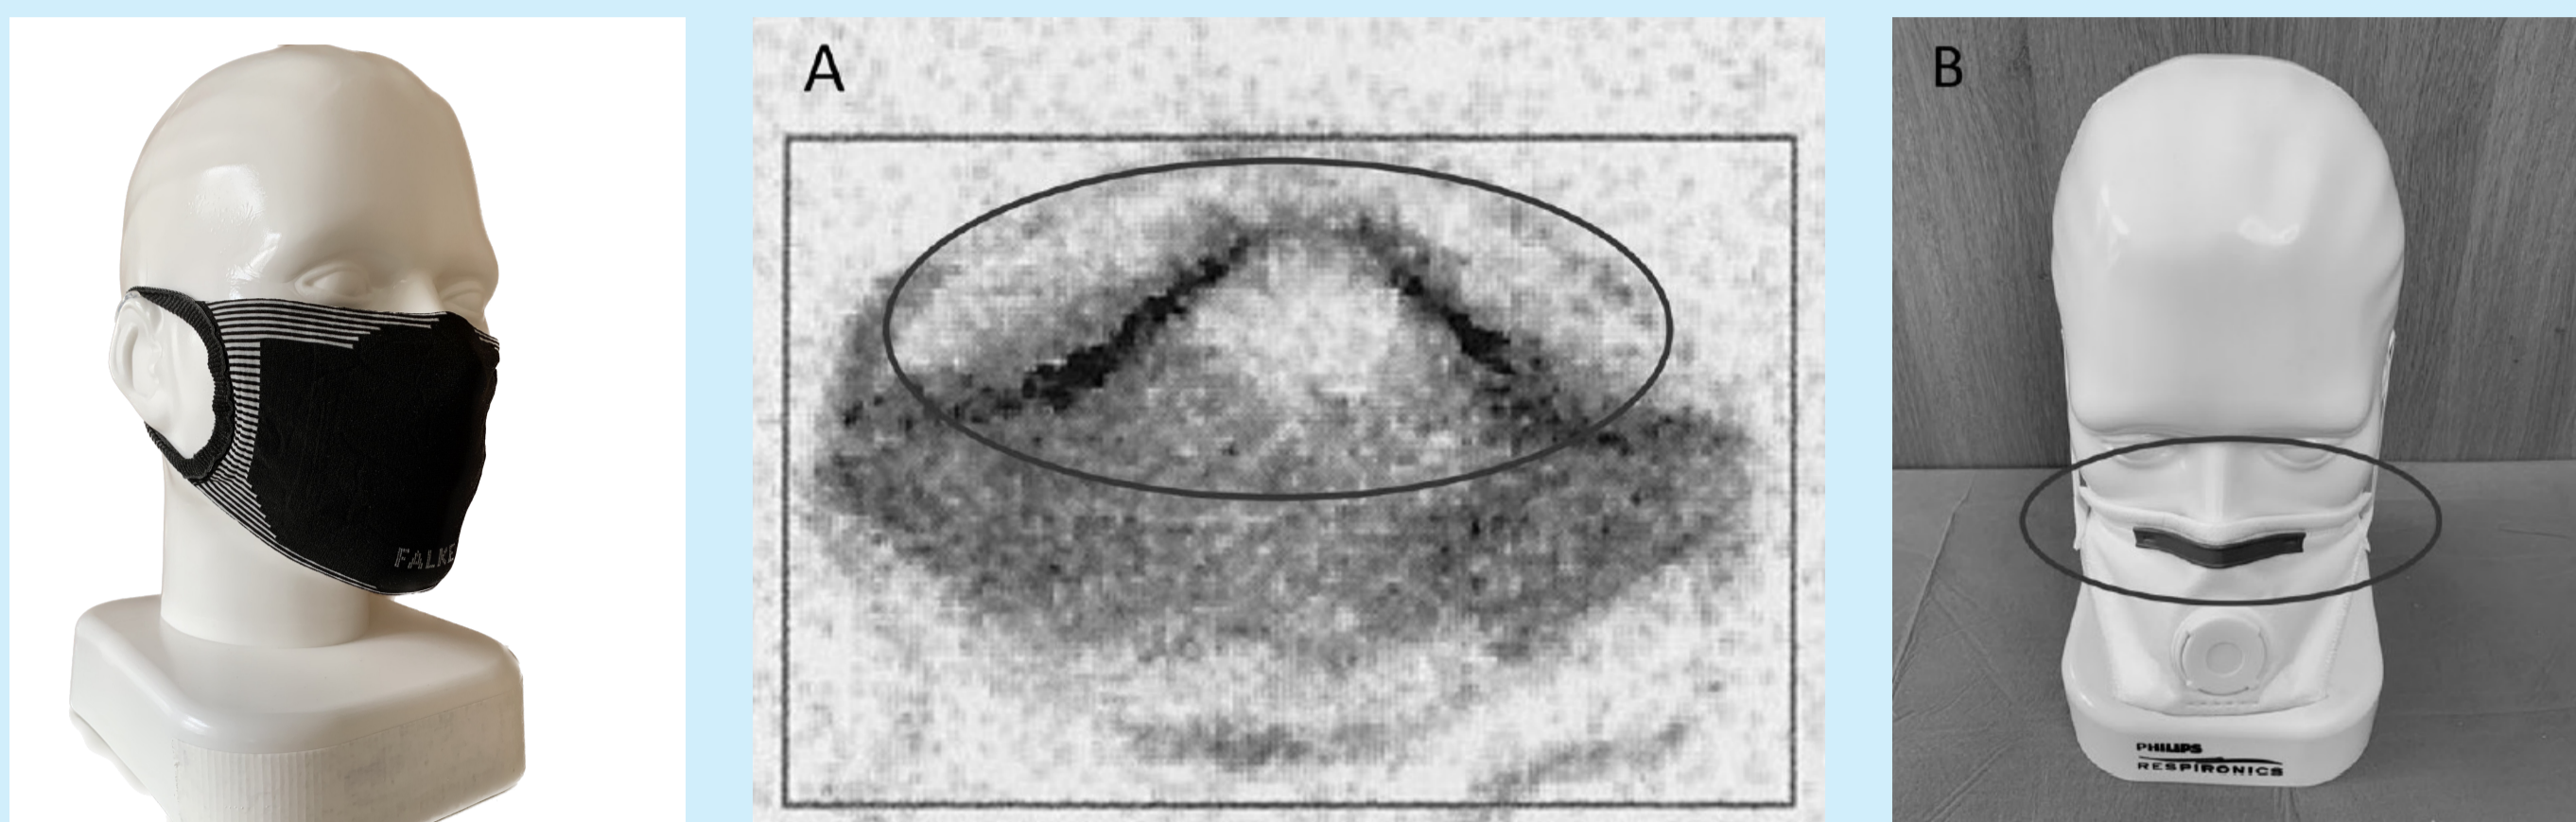



Corona

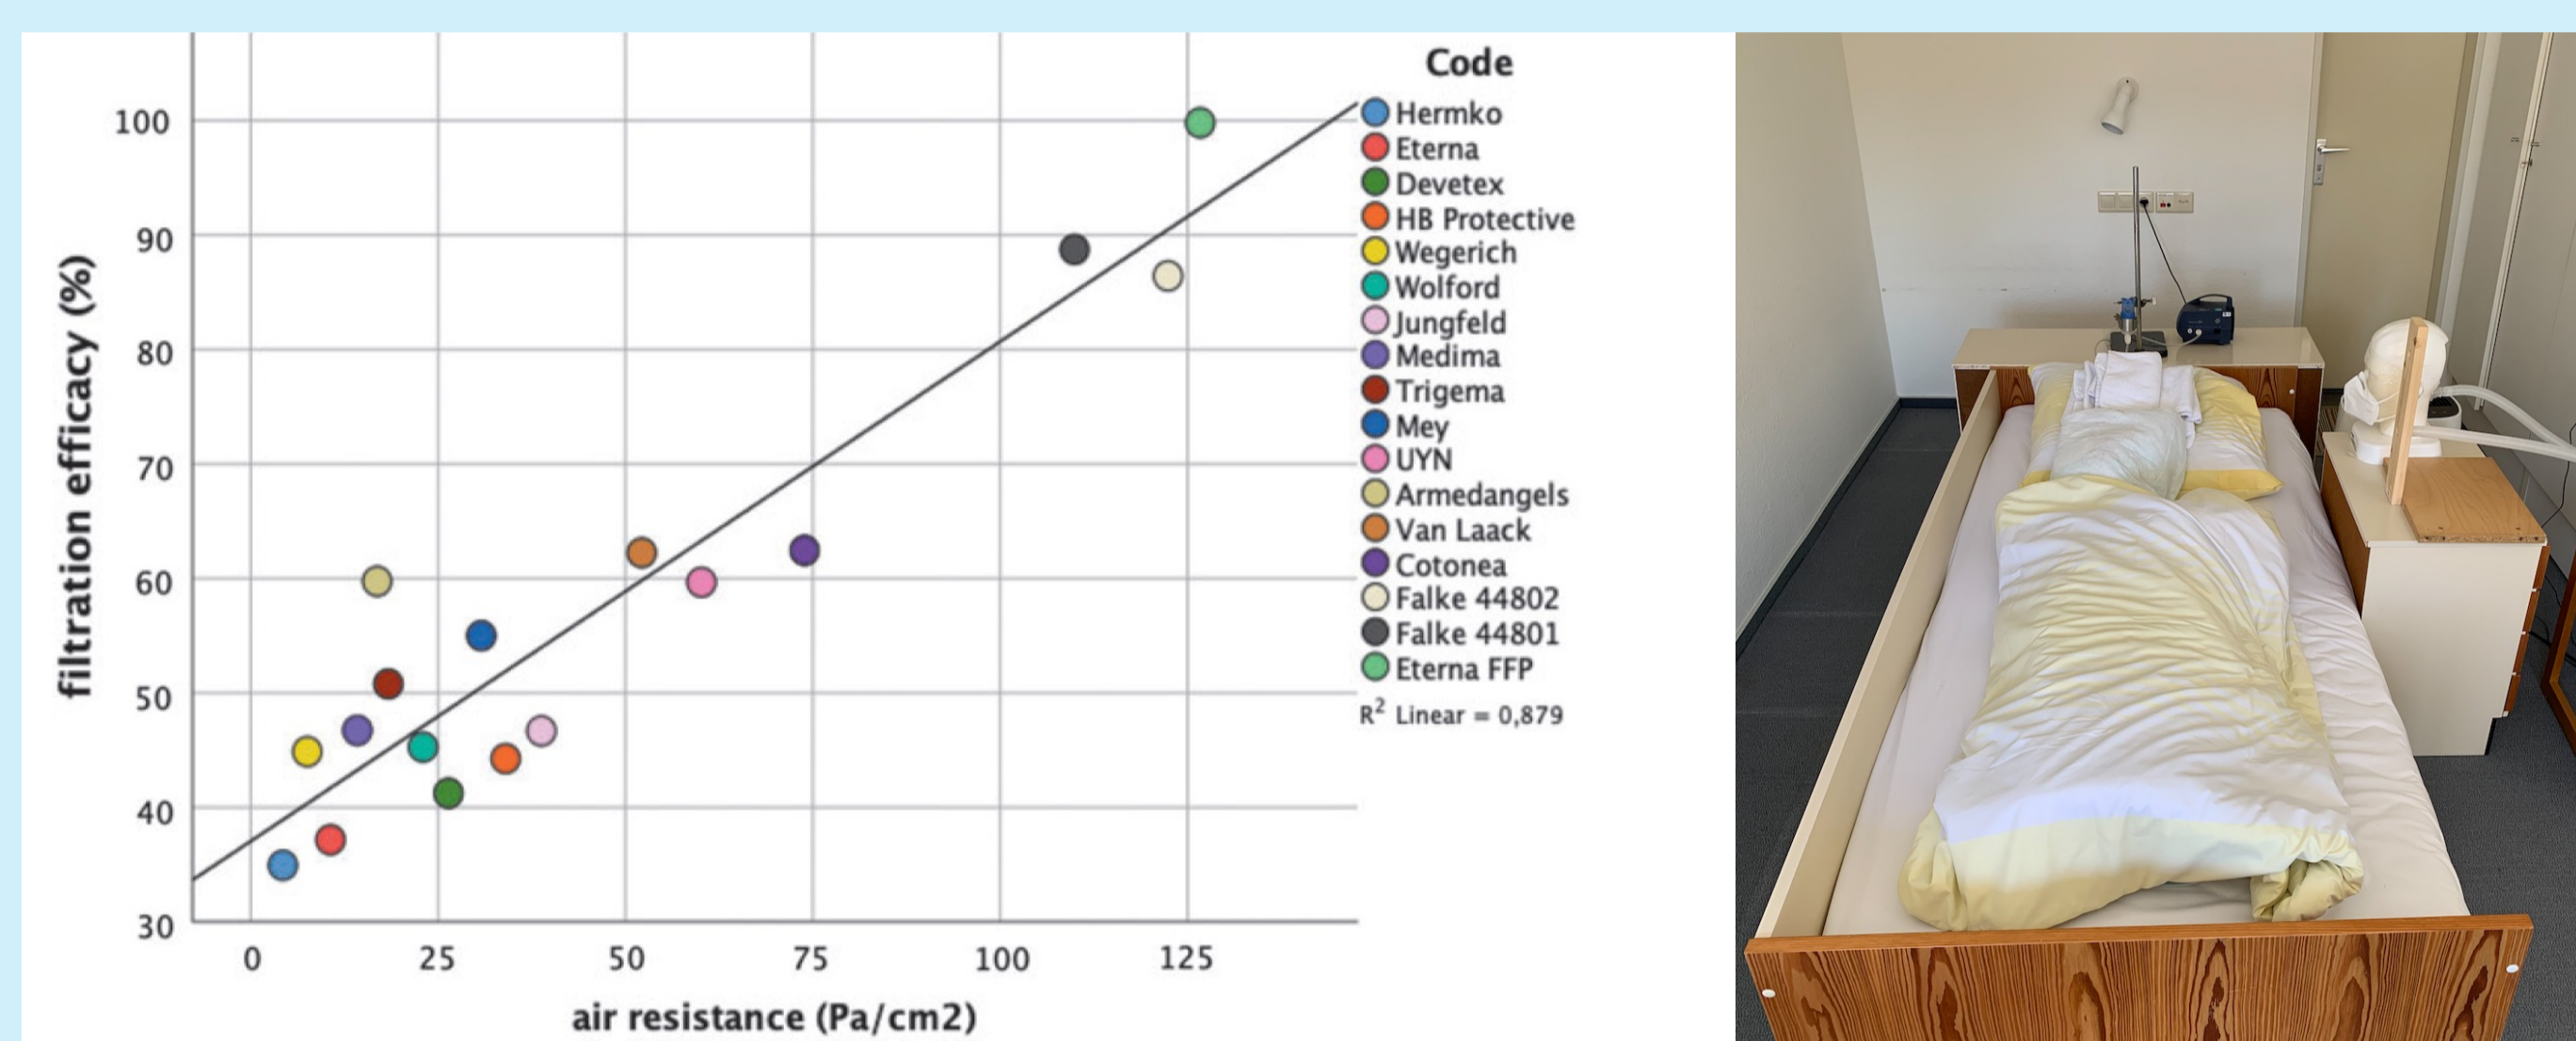

Increased radioactivity is seen around the upper edge of the respirator indicating leak flow in this area (A: scintigraphic image of the mounted mask (B)).

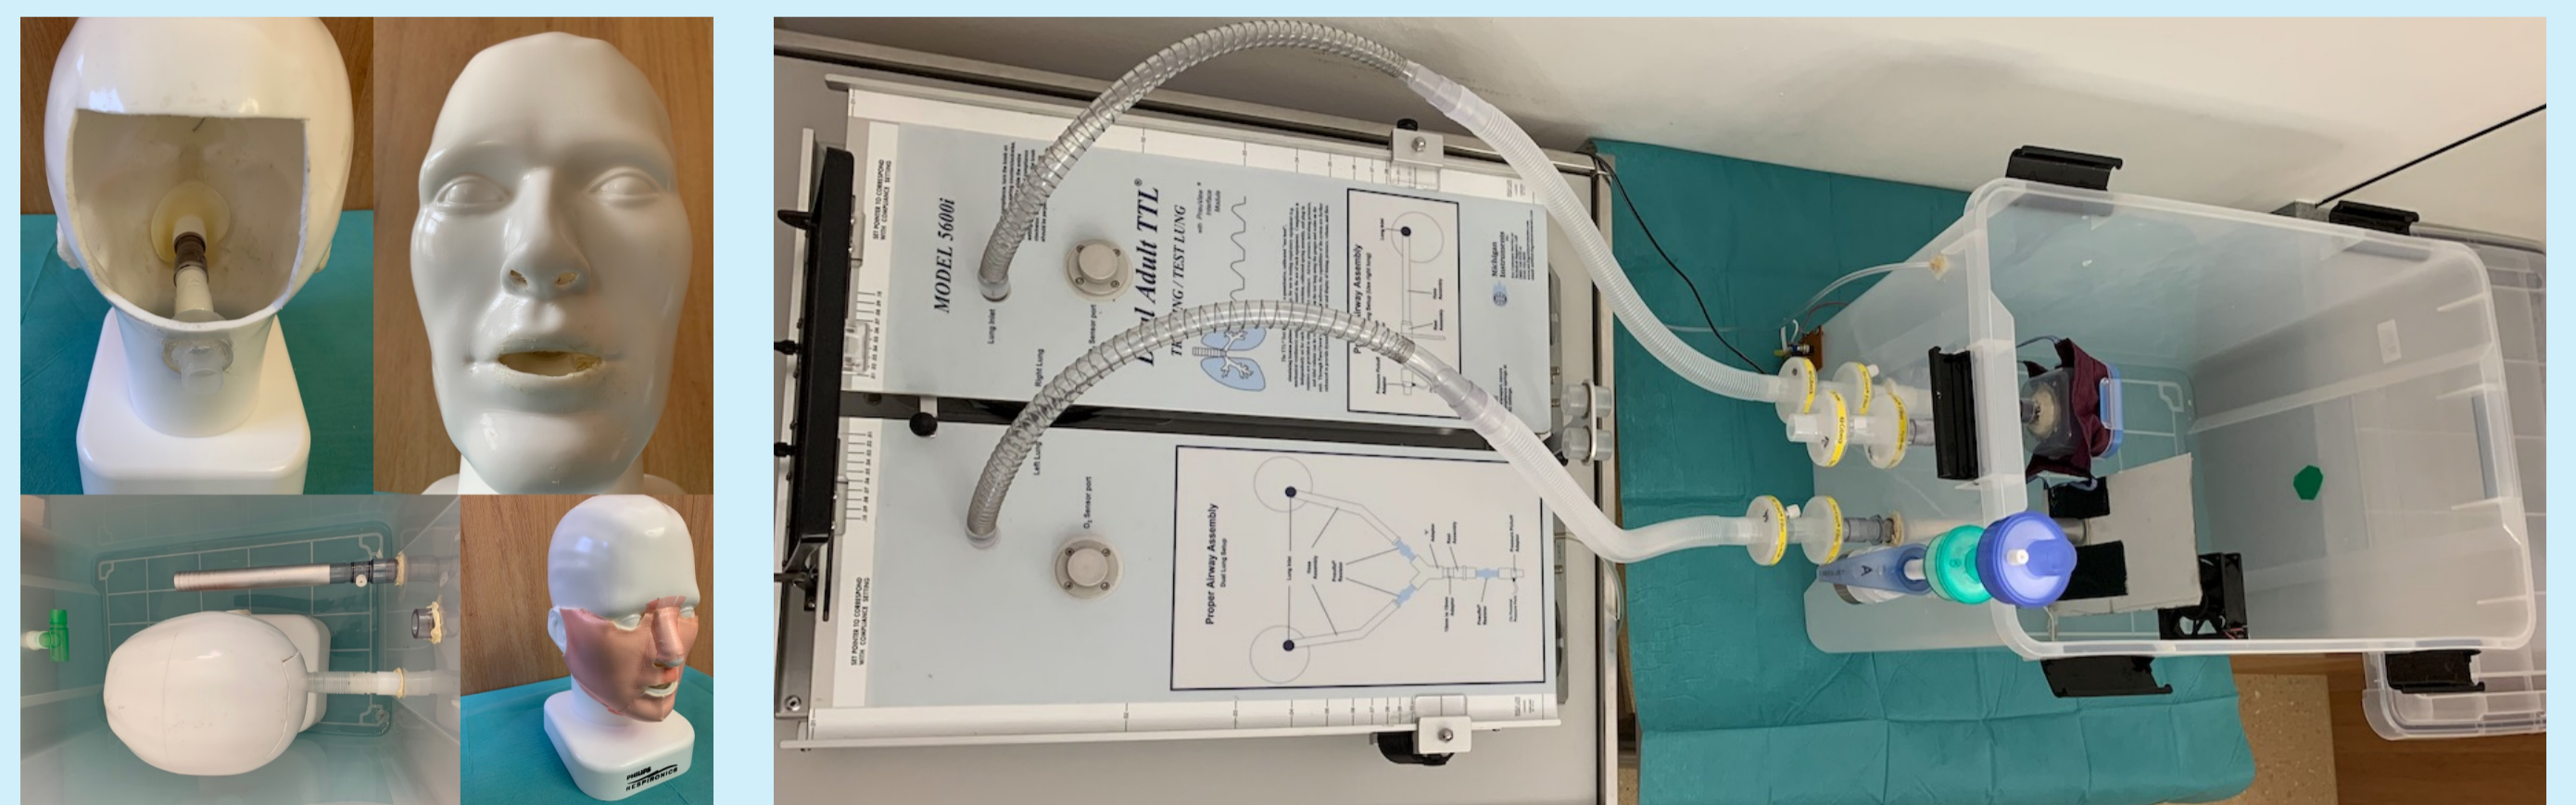

Filtration efficacy in % versus air resistance in Pascal/cm²

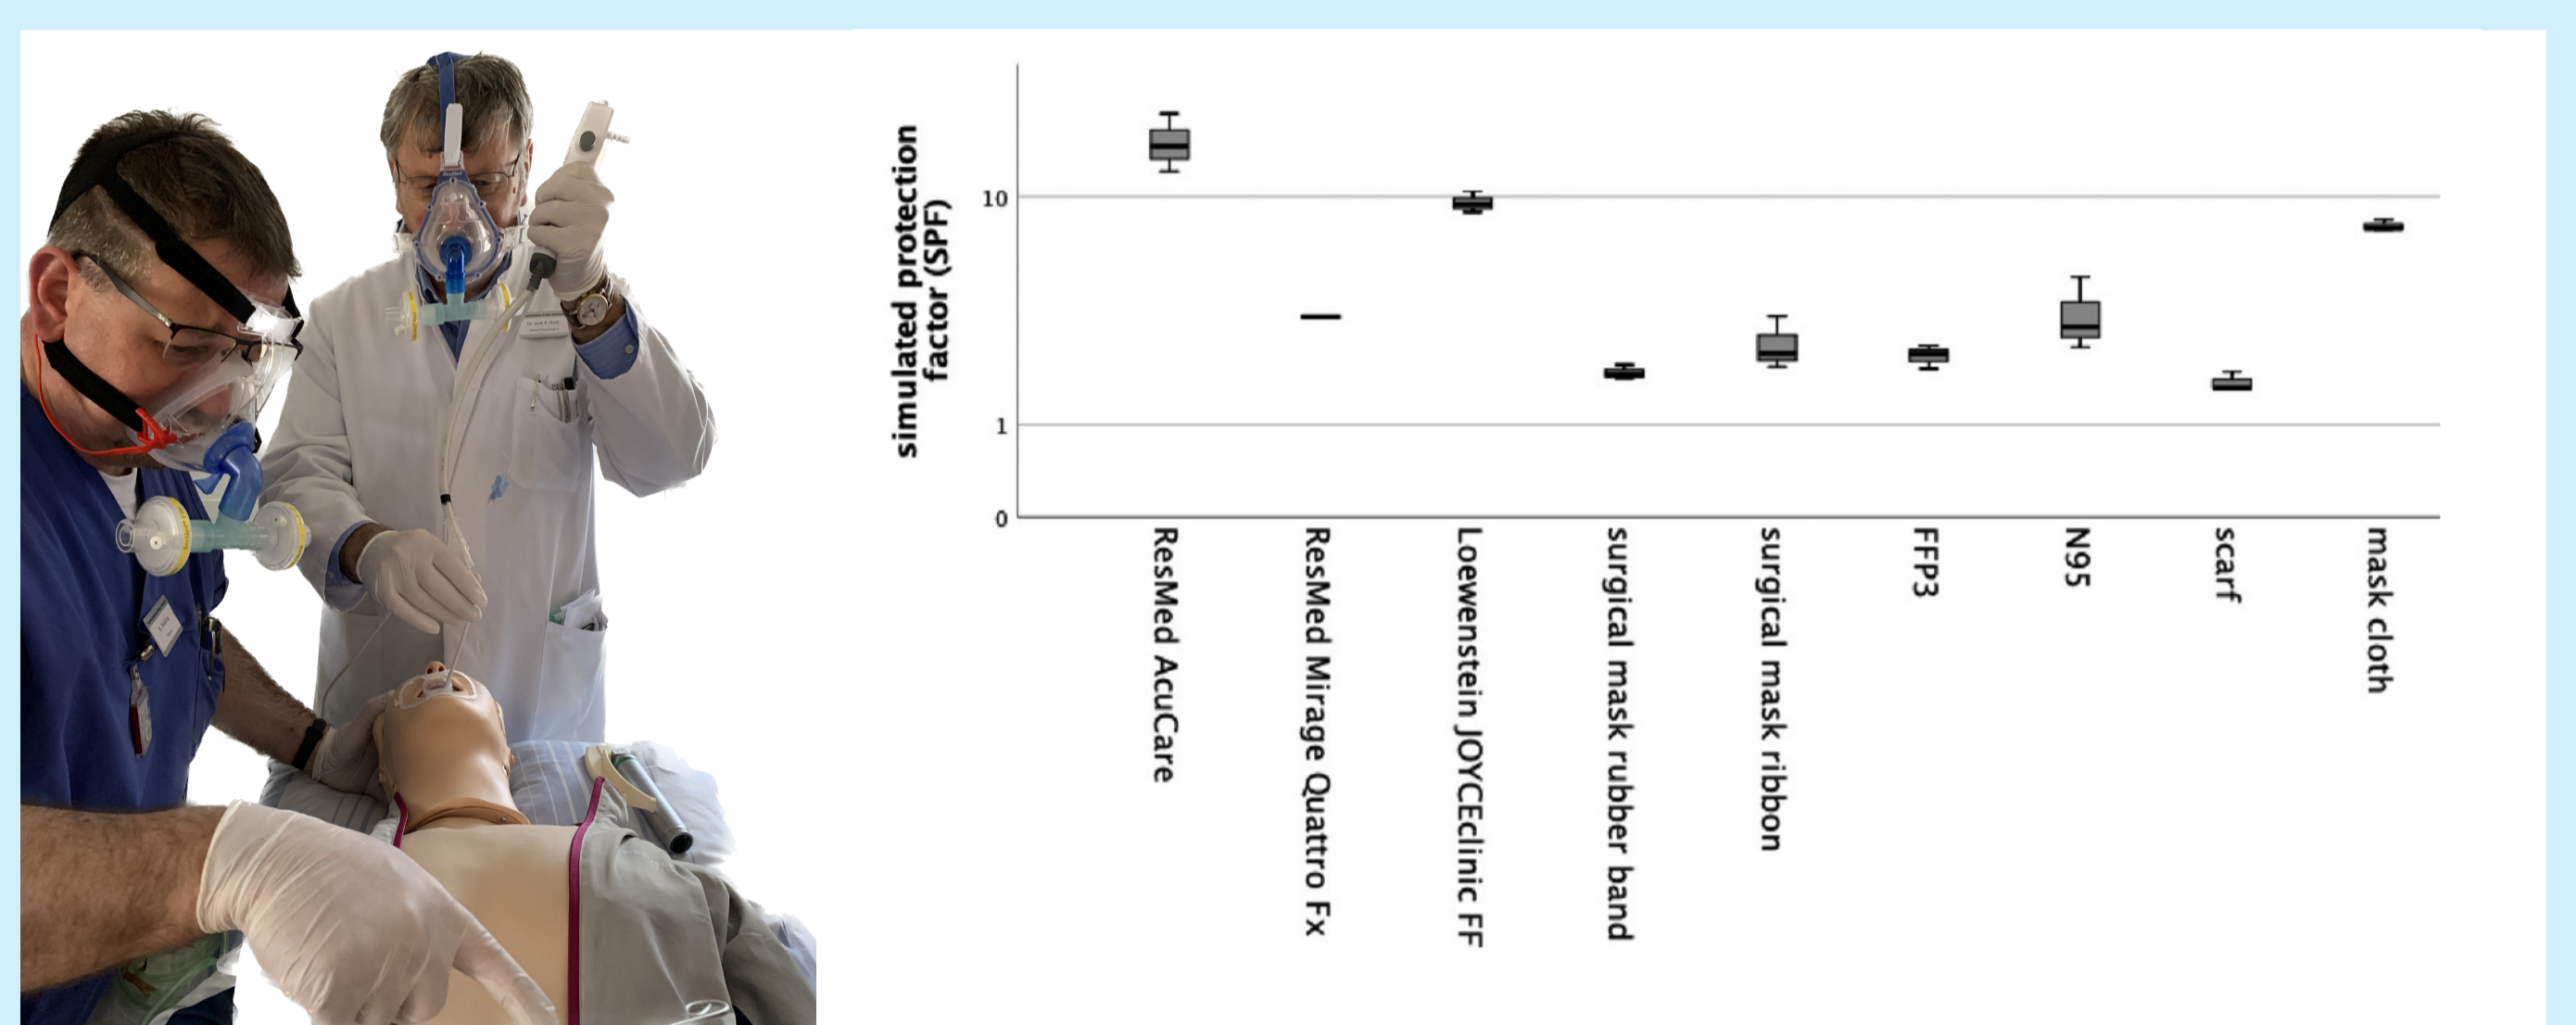

CEN
TC
205
WG17

DIN
AK
WG3

Continuous CO₂ levels over time for 1 individual with 15 min of data for each group. NIOSH exposure limit thresholds added for reference.

pius
HOSPITAL
Universitätsmedizin Oldenburg

LÖWENSTEIN
medical

MAX-PLANCK-INSTITUT
FÜR MULTIDISZIPLINÄRE NATURWISSENSCHAFTEN

Kostenkalkulation (INEK) Entwicklung von Prädiktoren


CT Scan
DICOM data

Planungssoftware
Prepare for the procedure

Navigate with LungGPS™
Technology
Navigate, biopsy, localize, prepare for treatment

Dyspnoe

Task Force Respiratory Failure Unit

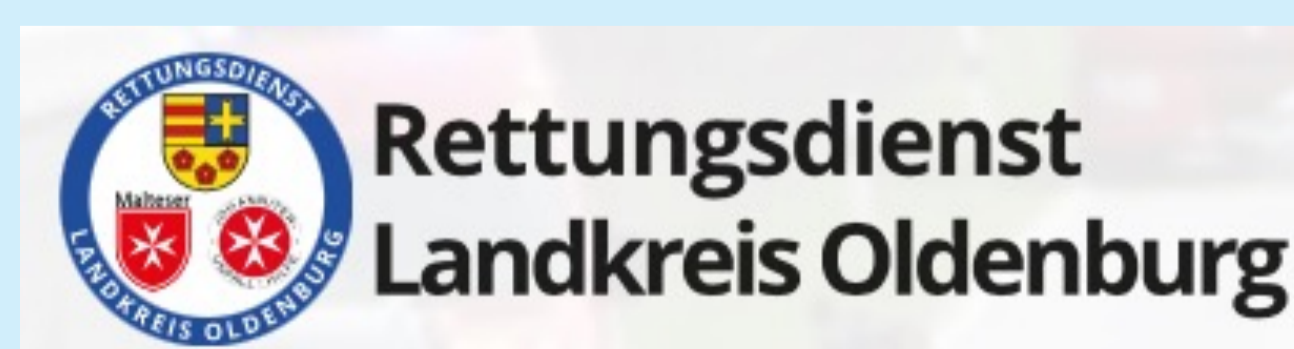

Fk. VI | Department für Versorgungsforschung
 Big Data in der Medizin

